



External Hex



PROVATA®





Drill Usage Guide

Tapered Drills


Ø3.0

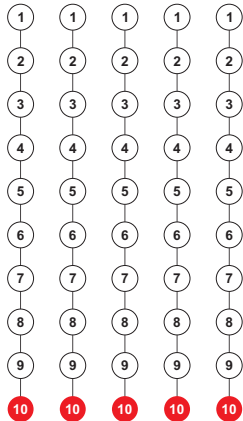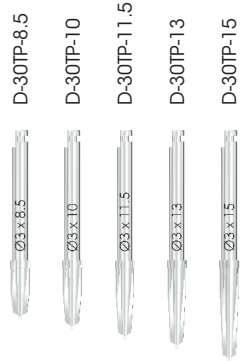



Ø3.3

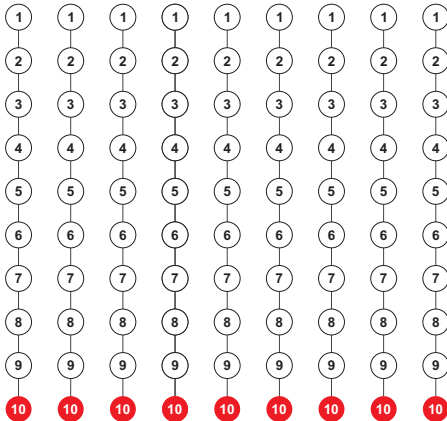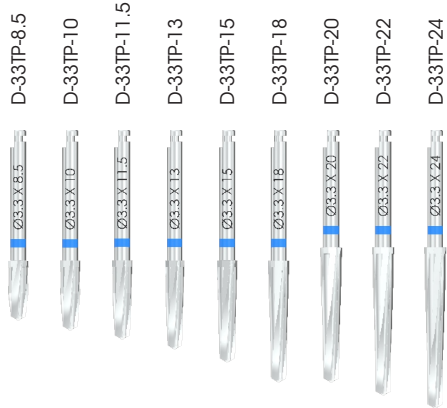



Ø4.0

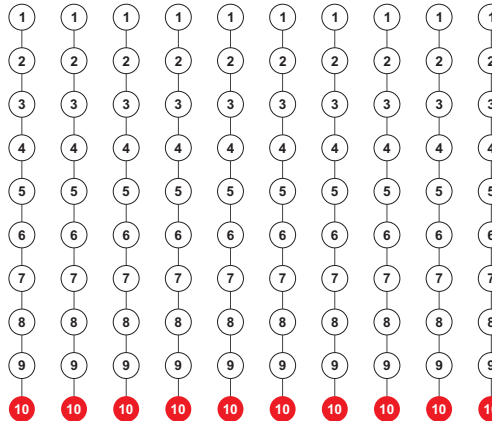

Ø5.0

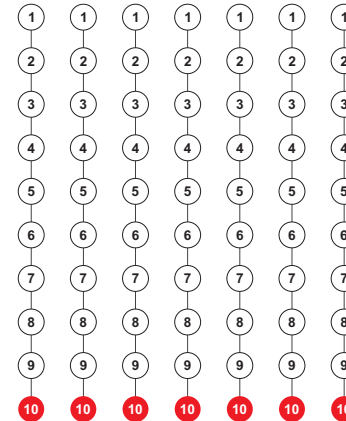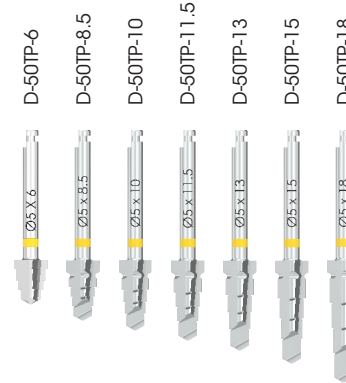

Ø6.0

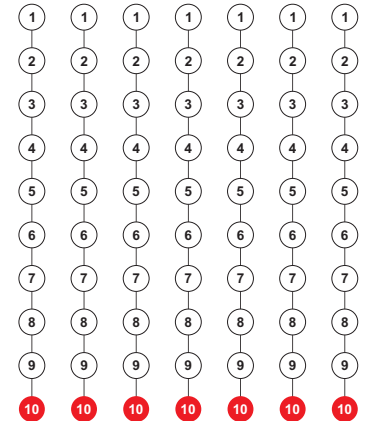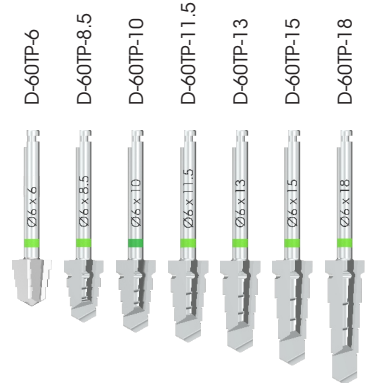

Our implant drills are made of hardened Surgical Stainless Steel OR Grade 5 Titanium. These drills can be reused, provided that they are cleaned adequately and resterilised. The cutting edge however does deteriorate with the number of usages and this is dependent on the hardness of bone, which has great variability. The tapered drills can be used for preparation of 10 implant sites without significant deterioration. However if any damage to the cutting edge of the drill is present, or if it appears to be blunt then it should be replaced.

Images are for illustration purposes only and do not necessarily accurately represent the product.

CAT-3114-02



External Hex


PROVATA®




Hard Bone Drill Usage Guide

Tapered Drills



Ø4.2

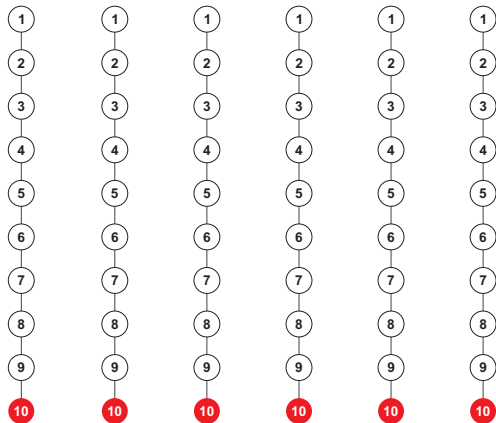



Ø5.2

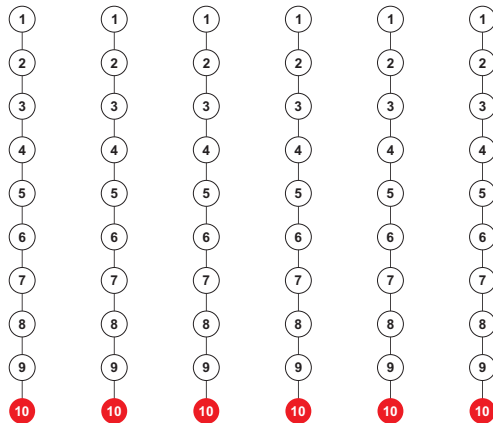

Ø6.2

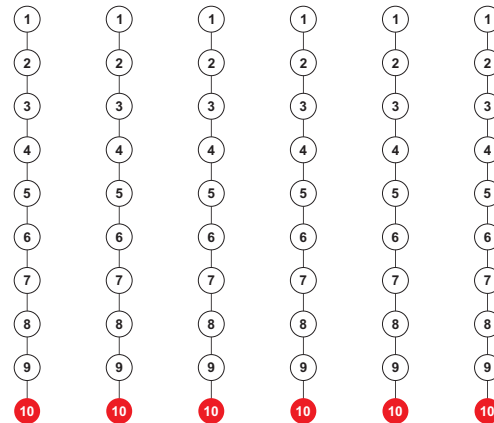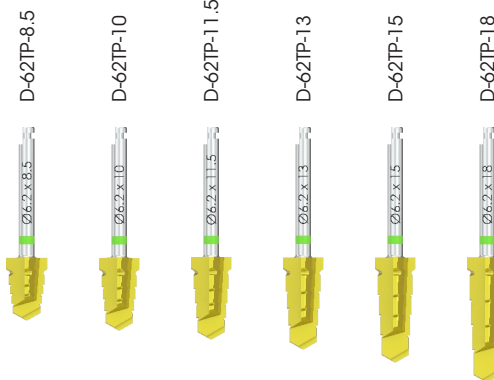

Taps

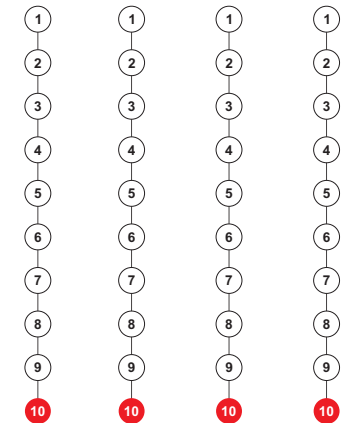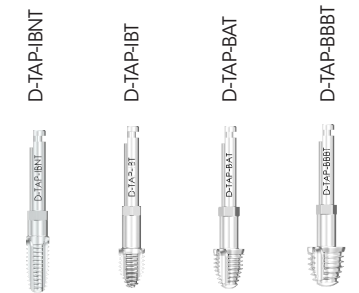

Our implant drills are made of hardened Surgical Stainless Steel OR Grade 5 Titanium. These drills can be reused, provided that they are cleaned adequately and resterilised. The cutting edge however does deteriorate with the number of usages and this is dependent on the hardness of bone, which has great variability. The tapered drills can be used for preparation of 10 implant sites without significant deterioration. However if any damage to the cutting edge of the drill is present, or if it appears to be blunt then it should be replaced.

Images are for illustration purposes only and do not necessarily accurately represent the product.